



AMMONIA

DETERMINATION OF AMMONIA IN PLASMA

Enzymatic method

Suitable for all analyzers – 300 tests


Product insert with instructions for automated and manual procedures

Stability > 4 years after production


Ammonia standard and controls included



Settings for automatic analyzers



Manual procedure

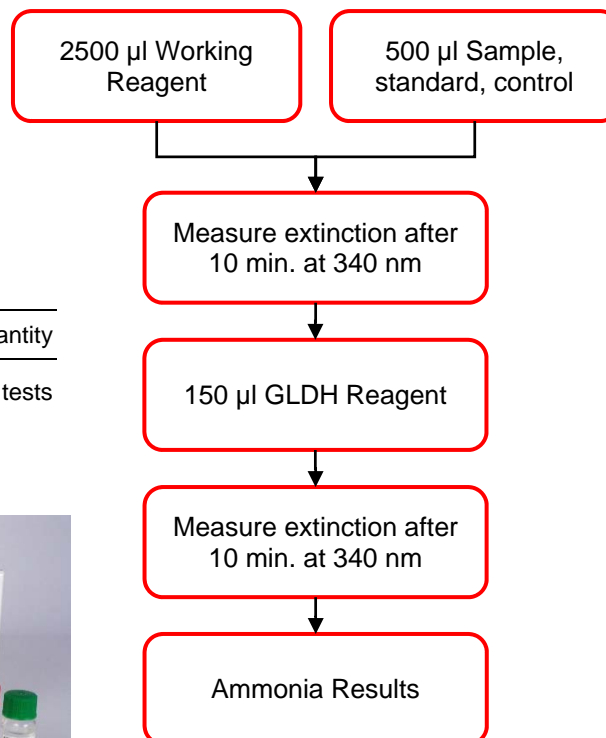

Product name	Product no.	Quantity
Ammonia Reagent Set (NADPH Method)	2230	24 - 300 tests





AMMONIA

DETERMINATION OF AMMONIA IN PLASMA


- Enzymatic method
- Suitable for all analyzers – 300 tests
- Product insert with instructions for automated and manual procedures
- Stability > 4 years after production
- Ammonia calibrator and controls included
- Wavelength 340 nm



Products	Product no.	Quantity
Ammonia Reagent Set	2230	24 manual 300 automated

SUMMARY

ASSAY PRINCIPLE



SAMPLE MATERIAL

Use venous EDTA blood collected without a tourniquet

LINEARITY

Up to 530 $\mu\text{mol/l}$

EXPECTED VALUES

6.5 - 45 $\mu\text{mol/l}$

QUALITY CONTROL

Products	Product no.	Quantity
Ammonia Control Normal Level	2984	1 x 5 ml
Ammonia Control High Level	2229	1 x 5 ml

QUANTITY OF DETERMINATIONS

According to product insert of Ammonia Reagent Set (2230):

Procedure

- Manual : 24 tests
- Automated : 300 tests

NOTES

1. For in vitro diagnostic use only.
2. For professional use only.
3. Always contact INstru**chemie** for the complete product insert and latest edition.
4. Printed in the Netherlands, July 2015, edition 2.0