





## PHOSPHOLIPIDS

### DETERMINATION OF PHOSPHOLIPIDS IN SERUM OR PLASMA

- Enzymatic method
- Liquid, ready for use reagent
- For Manual and/or Automated Procedures
- Use Serum or Plasma
- Also available Phospholipids Calibrator & Controls
- Wavelength 505 nm



Products	Product no.	Quantity
Phospholipids Reagent Set	3009	50 manual 160 automated
Phospholipids Calibrator	3012	1 x 2 ml
Phospholipids Control Low Level	3013	10 x 1 ml
Phospholipids Control Normal Level	3014	10 x 1 ml
Phospholipids Control High Level	3015	10 x 1 ml

## SUMMARY

### ASSAY PRINCIPLE

Phospholipids (Lecithin, Lysolecithin, Sphingomyelin) + H<sub>2</sub>O  $\xrightarrow{\text{Phospholipase D}}$  Choline + Phosphatidic Acid

2 Choline + 2 O<sub>2</sub>  $\xrightarrow{\text{Choline Oxidase}}$  2 H<sub>2</sub>O<sub>2</sub> + Betaine

4 – Aminoantipyrine + Phenol + 2 H<sub>2</sub>O<sub>2</sub>  $\xrightarrow{\text{Peroxidase}}$  Red Quinone Pigment Chromogen + 4 H<sub>2</sub>O

### SAMPLE MATERIAL

Serum or Plasma (Heparin or EDTA).

### LINEARITY

Up to 7.00 mmol/l

### EXPECTED VALUES

Serum or Heparinized Plasma - Normal: 1.94 – 3.23 mmol/l at 37°C

### QUALITY CONTROLS

Products	Product no.	Quantity
Phospholipids Control Low Level	3013	10 x 1 ml
Phospholipids Control Normal Level	3014	10 x 1 ml
Phospholipids Control High Level	3015	10 x 1 ml

### QUANTITY OF DETERMINATIONS

According to product insert of Phospholipids Reagent Set (3009):

Procedure

- Manual : 50 tests
- Automated : 160 tests

### NOTES

1. For in vitro diagnostic use only.
2. For professional use only.
3. Always contact INstruChemie for the complete product insert and latest edition.
4. Printed in the Netherlands, January 2015, version 3.0



## CONCENTRATION MEASUREMENTS

The concentrations of a low, normal and high human serum were measured manually with a spectrophotometer.

### Phospholipids measurements

	Low	Normal	High
Extinction	0.1166	0.3766	0.9705
Concentration (mmol/l)	0.99	2.96	7.64

## TEST CONDITIONS

All tests were conducted under the following conditions:

Temperature	: 37 °C
Wavelength	: 505 nm
Light path	: Analyzer: 0.7 cm / Manual: 1.0 cm
Blanc	: Reagent blank
Sample	: Serum

## SENSITIVITY


The sensitivity (limit of detection) was determined by measuring human control material 20 times (Phospholipids activity = 0 mmol/l).

$$\text{Sensitivity} = 3x \text{ standard deviation} = 3x 0.0061 = 0.018 \text{ mmol/l}$$

## LINEARITY

The Phospholipids assay is linear up to 7.00 mmol/l.

### Linearity measurements with an automatic analyzer

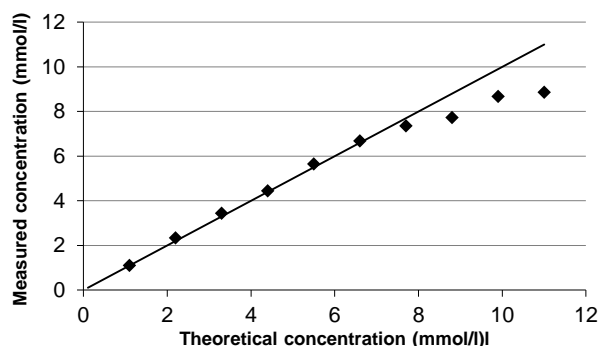

## RECOVERY

The recovery is determined by measuring the Phospholipids concentrations of spiked human sera 10 times using an automatic analyzer.

### Recovery:

Added Phospholipids (mmol/l)	Measured (mmol/l)	Recovery (%)
1.55	1.54	99.4
4.25	4.21	99.1
5.46	5.44	99.6

## PRECISION

The precision is determined by measuring a human serum and Phospholipids Calibrator 10 times a day (repeatability) for 5 consecutive days (reproducibility), using an automatic analyzer.

### Repeatability:

	Sample (mmol/l)	Calibrator (mmol/l)
Mean	3.12	4.06
Standard deviation	0.03	0.03
Variation coefficient	0.96	0.74


### Reproducibility:

	Sample (mmol/l)	Calibrator (mmol/l)
Mean	3.12	3.90
Standard deviation	0.03	0.03
Variation coefficient	0.96	0.77

## CORRELATION

Pearsons' correlation is determined by measuring the Phospholipids concentration in multiple human sera with reagent of INstruChemie and reagent from another manufacturer.

### Correlation measured with an automatic analyzer (mmol/l)

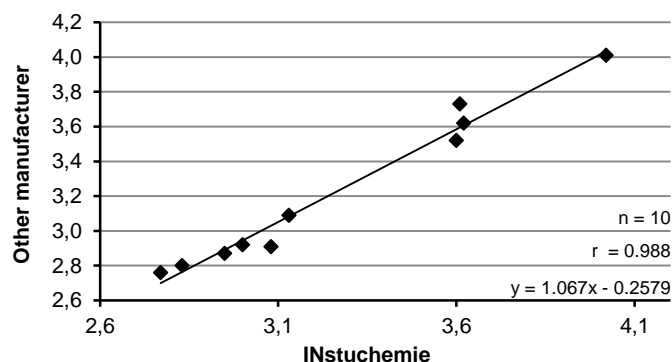

**FAX – FORM: +31-(0)596 – 634 755****TELEPHONE NO.: +31-(0)596 – 634 831****EMAIL: info@instruChemie.nl**

<b>Attn</b>	INstruChemie B.V. Sales & Marketing Fons Nieland, Arie Jan de Graaf
<b>Tel no.</b>	+31-(0)596 – 634 831
<b>Fax no.</b>	+31-(0)596 – 634 755
<b>E-mail</b>	info@instruChemie.nl
<b>Date</b>	February 2016
<b>Reference</b>	2150205-1.FEN

**I would like:**

<input type="checkbox"/>	<b>Personal contact.</b>	<b>About:</b>
--------------------------	--------------------------	---------------

<input type="checkbox"/>	<b>More information.</b>	<b>About:</b>
--------------------------	--------------------------	---------------

<input type="checkbox"/>	<b>Actual prices.</b>	<b>Of:</b>
--------------------------	-----------------------	------------

<input type="checkbox"/>	<b>Catalogue.</b>	
--------------------------	-------------------	--

**Send to:**

Name:			
Initials		Titel:	M / F
Function:			
Company/Lab:			
Department:			
Address:			
City:			
Telephone:			
Fax:			
E-mail:			